

Comparison of 1R6F and 3R4F Smoke and Tobacco Filler HPHC Means and Standard Deviations

Michael J. Morton, Tammy L. Blake, Karl A. Wagner

*Altria Client Services LLC, Richmond, VA 23219
Center for Research and Technology*

**74th Tobacco Science Research Conference
Boston, MA**

August 29 – September 1, 2021



2021_TSRC78_Morton.pdf
Presented by COPR STA
© 2021 Altria Client Services LLC

Reference Cigarettes

- Used for numerous purposes including:
 - Quality control monitors
 - Model cigarette systems
 - Analytical method development tools
 - Interlab study samples
- We used the 3R4F cigarette as our primary quality control monitor from 2015 to early 2021
- Because of limited remaining quantities of 3R4F, we transitioned to 1R6F as our primary quality control monitor in early 2021
- Both 1R6F and 3R4F were manufactured over several days and are subject to normal day-to-day manufacturing variation
 - Analyte levels can be somewhat different on different days of manufacture so comparisons can modestly differ depending on which batches are being compared

Blend and Design Information

Component	3R4F	1R6F
Flue Cured	35.4%	34%
Burley	21.6%	24%
Maryland	1.4%	0%
Oriental	12.1%	12%
Reconstituted Tobacco	29.6%	20%
Expanded FC	0%	7%
Expanded Burley	0%	3%
Glycerin	2.7%	1.7%
Propylene Glycol	0.0%	1.0%
Isosweet (Sugar)	6.4%	6.3%

Characteristic	3R4F	1R6F
Cigarette Length	84 mm	83 mm
Tobacco Rod Circ.	24.8 mm	24.8 mm
Tobacco rod Length	57 mm	56 mm
Filter Length	27 mm	27 mm
Tobacco Weight	0.783 g	0.640 g
Cigarette Weight	1.06 g	0.887 g
Total RTD	128 mm	107 mm
Plug RTD	115 mm	99 mm
Ventilation	30%	30%
Paper Permeability	24 CU	46 CU
Paper Citrate	0.60%	0.60%
Cigarette Paper	Non-Banded	Banded
Manufacture Period	Dec 2006	Mar 2015

Tar Nicotine and CO comparison

	Analyte	1R6F Mean	3R4F Mean	1R6F Std	3R4F Std	1R6F N	3R4F N
Non-Intense ISO 3308	CO	10.0	10.7	0.64	0.61	263	159
	Nicotine	0.72	0.73	0.03	0.03	263	159
	TPM	10.3	10.1	0.43	0.46	263	159
	Tar	8.8	8.5	0.35	0.39	263	159
	Puff Count	7.88	8.32	0.24	0.24	263	159
	Water	0.80	0.85	0.08	0.09	263	159
Intense ISO 20778	CO	28.6	31.0	1.61	1.73	267	160
	Nicotine	2.00	2.00	0.09	0.11	267	160
	TPM	47.9	46.7	2.84	2.73	267	160
	Tar	29.2	28.5	1.54	1.52	267	160
	Puff Count	9.09	10.43	0.38	0.42	267	160
	Water	16.7	16.3	1.51	1.62	267	160

Methods Using 3R4F/1R6F as a Monitor


Filler/Tobacco Methods*	Smoke Methods
Ammonia	Aromatic Amines
Nicotine and minor alkaloids	Carbonyls
TSNAs	B(a)P
B(a)P	VOCs
Metals	TSNAs
Nitrate/Nitrite	

* Filler methods were based on large ground composite samples.

Parallel Testing Scheme


- For smoke runs
 - 2 ports each 3R4F and 1R6F per 20-port linear smoke run
 - Non-intense (ISO 3308) and Intense (ISO 20778)
- For tobacco runs
 - 2 or 3 reps of 3R4F and 1R6F in each tobacco sequence
 - Both fillers were from homogenized batches
- Data were collected for each method for at least 10 months

3R4F/1R6F Filler Comparisons

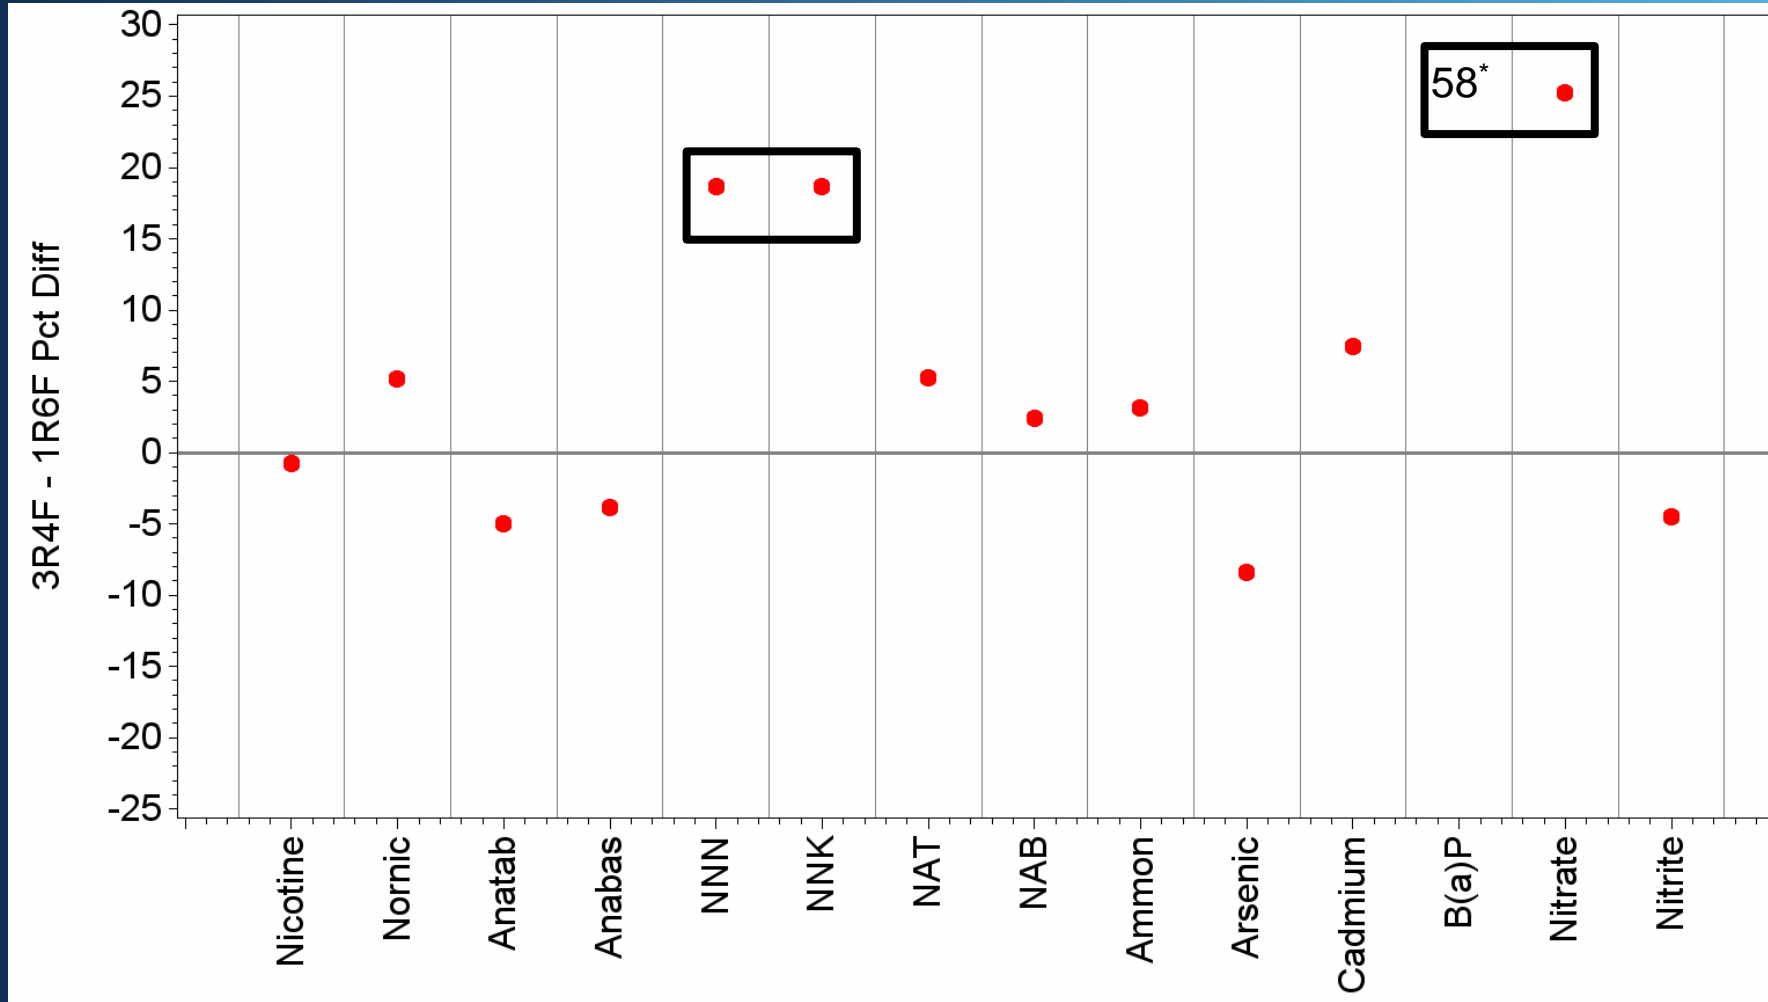


*Note the B(a)P value is beyond the scale of the graph and the value=58 is shown in text.

3R4F/1R6F Filler NNN

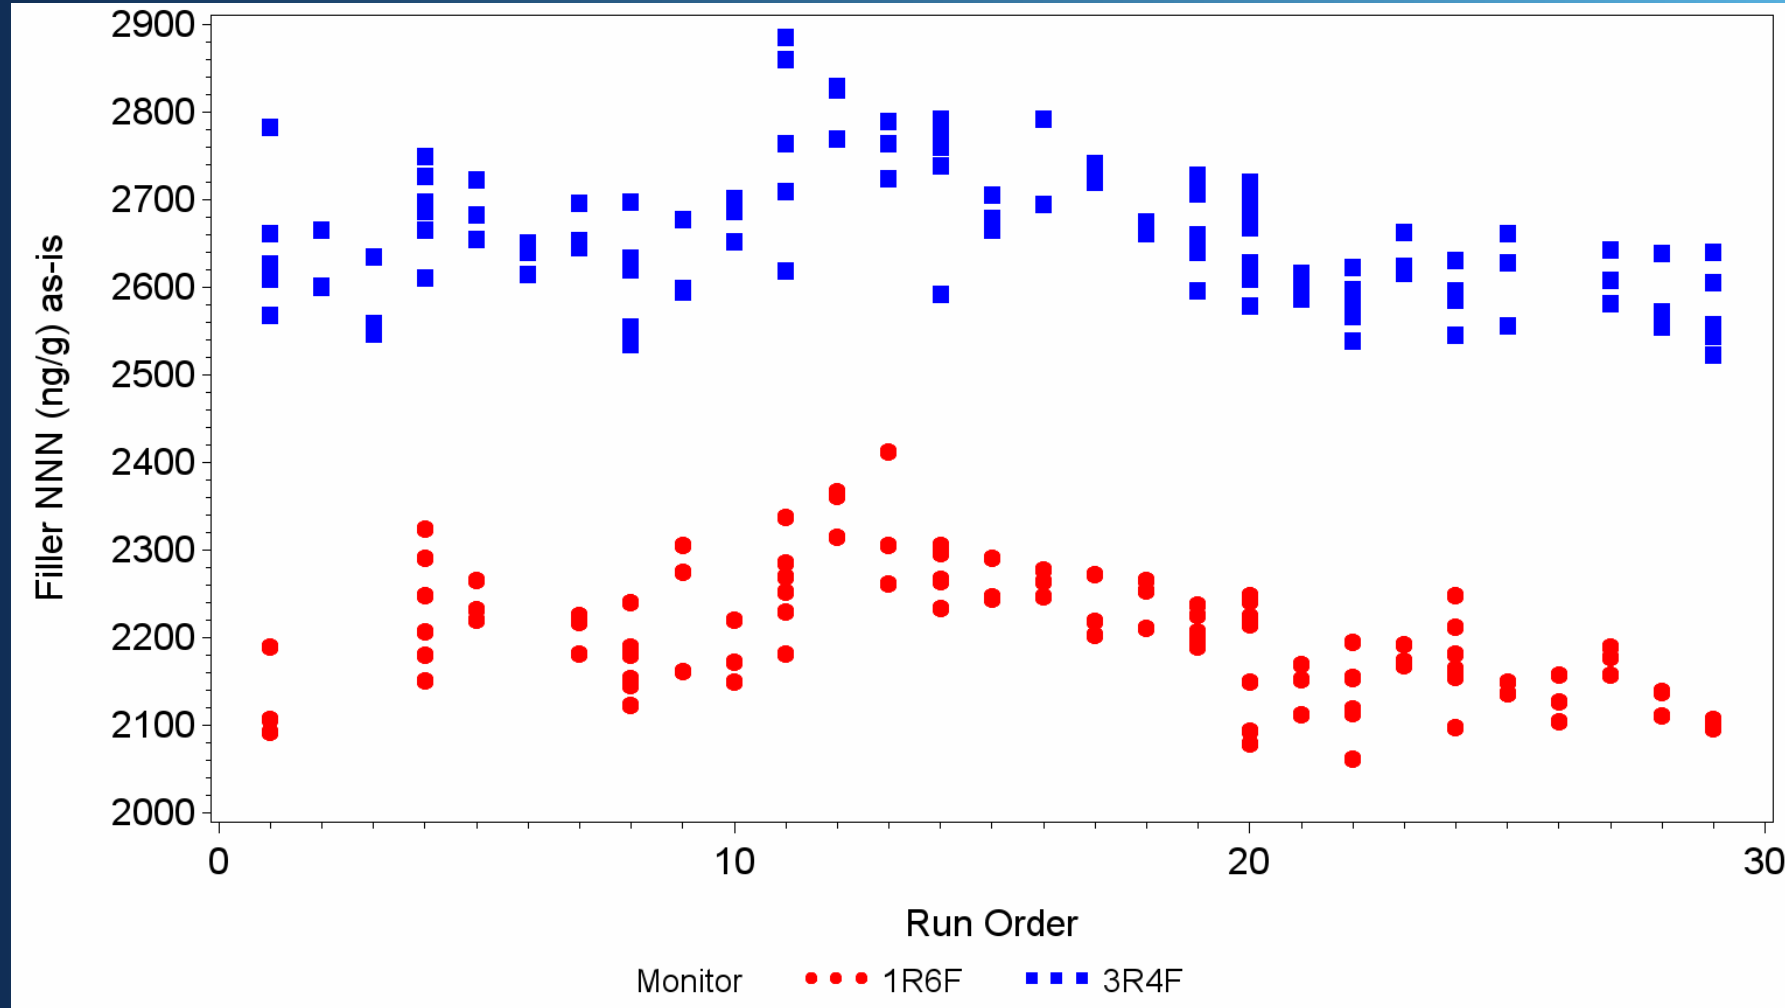


The cigarettes were made more than 8 years apart and TSNAs are known to show large year-to-year variability.


3R4F/1R6F Filler Nicotine

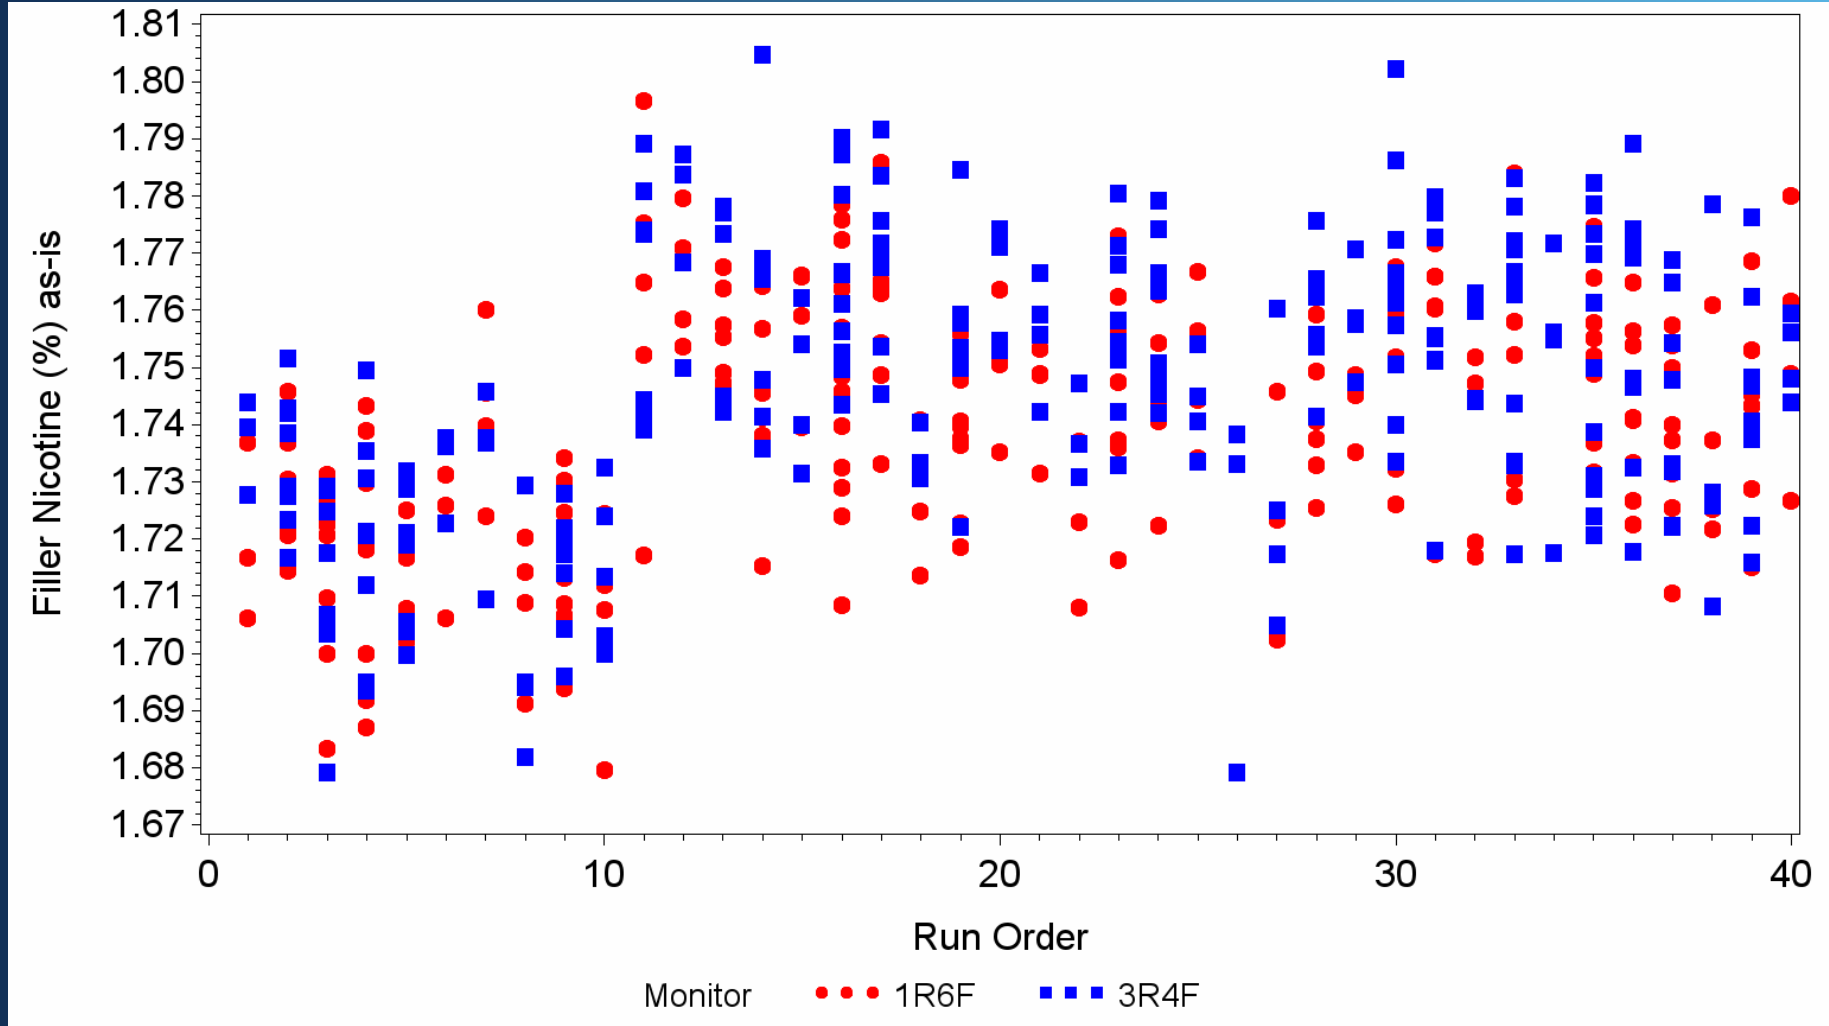

3R4F/1R6F Filler B(a)P

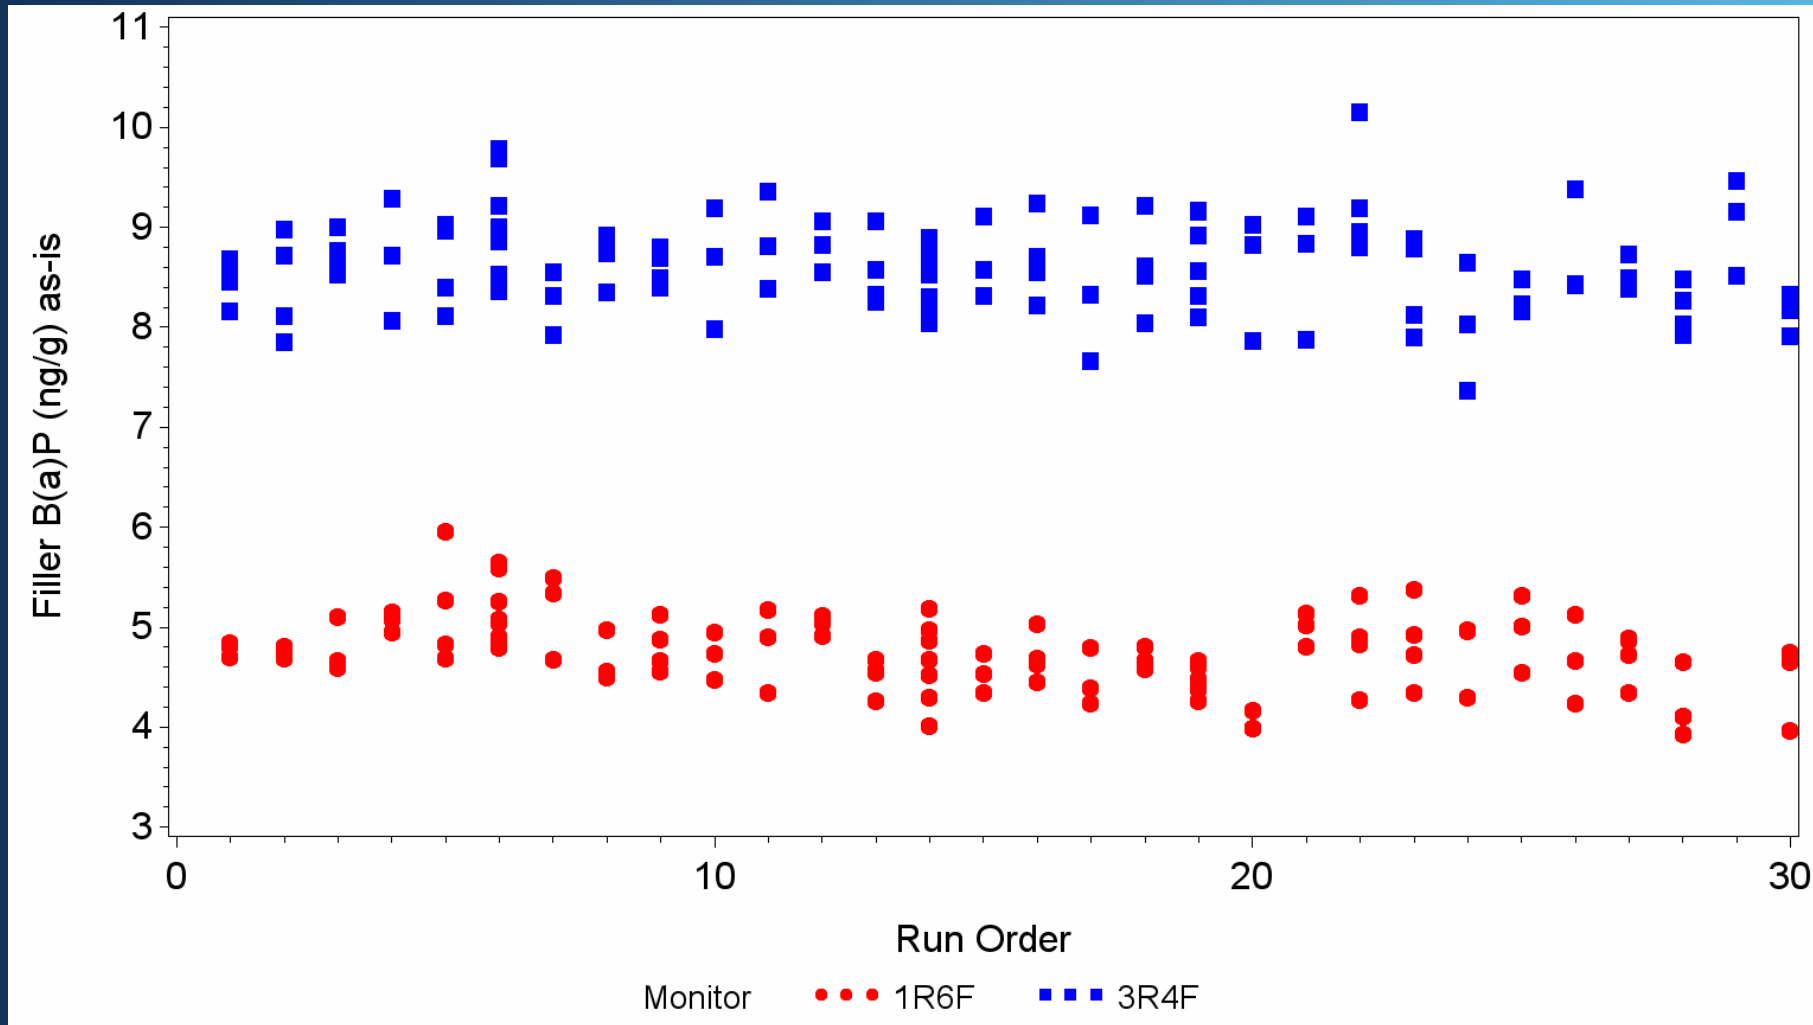


3R4F/1R6F Smoke Comparisons

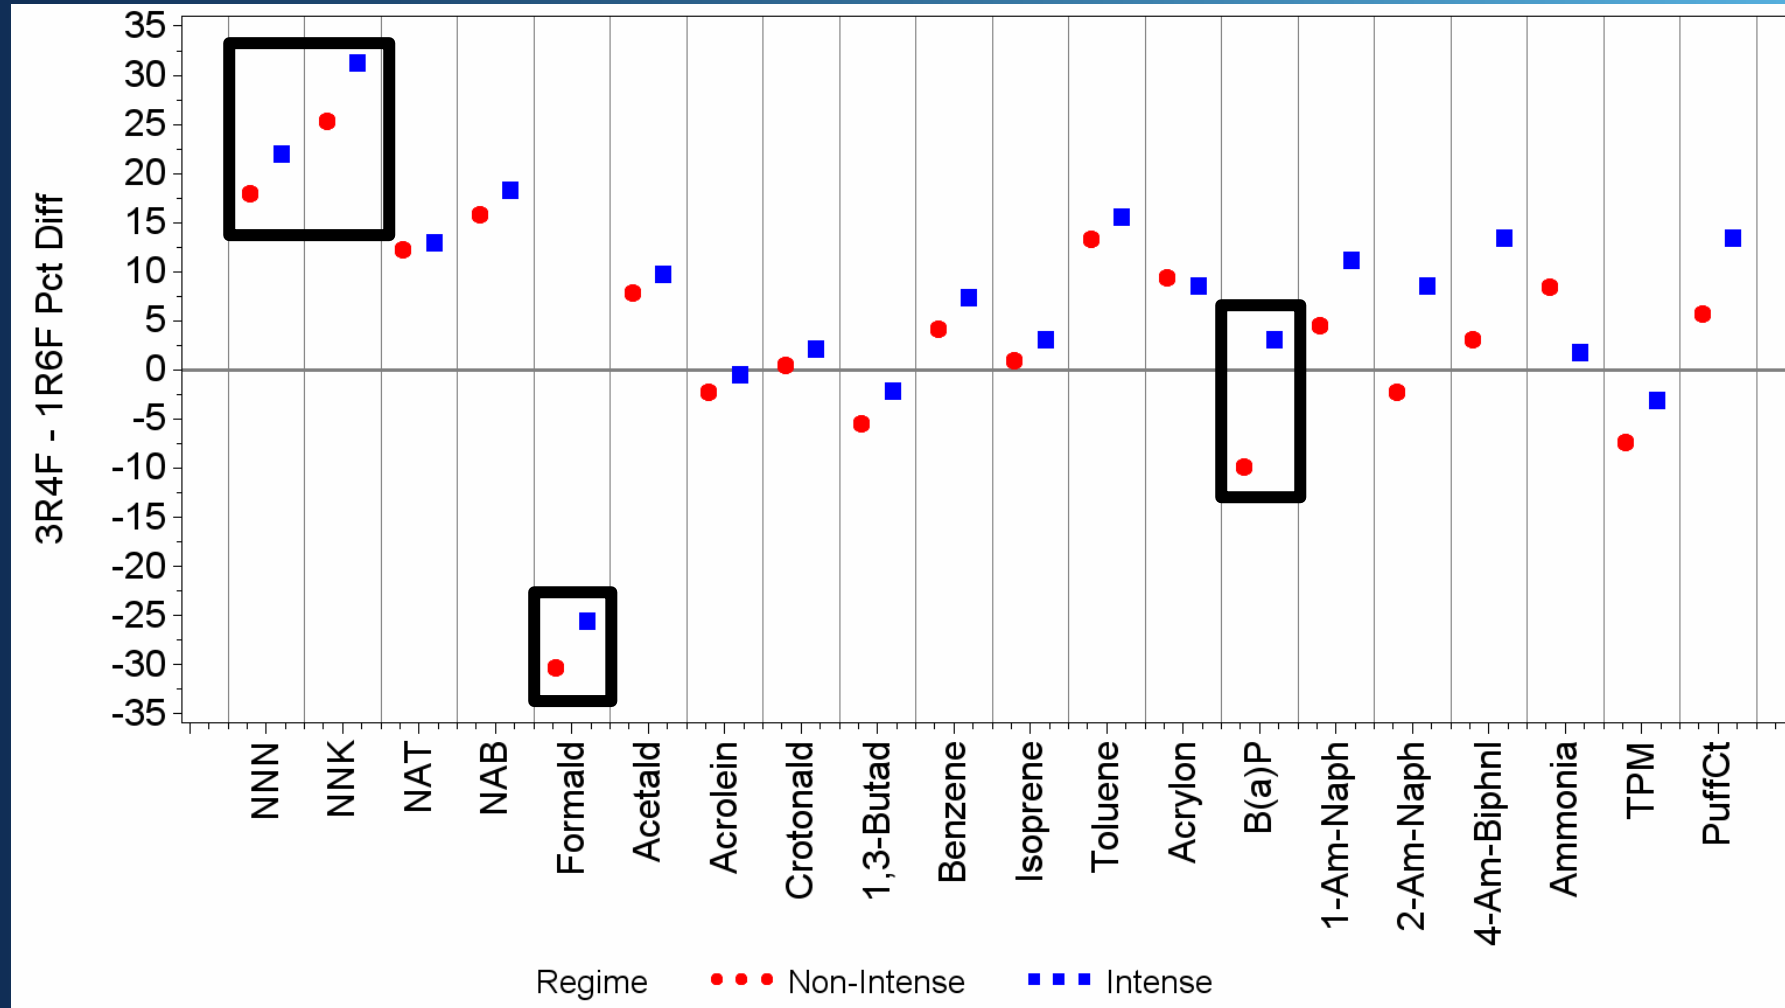


NNN and NNK show a similar trend as was seen with the filler

The B(a)P difference is small despite the filler differences


NNN in Smoke – Intense

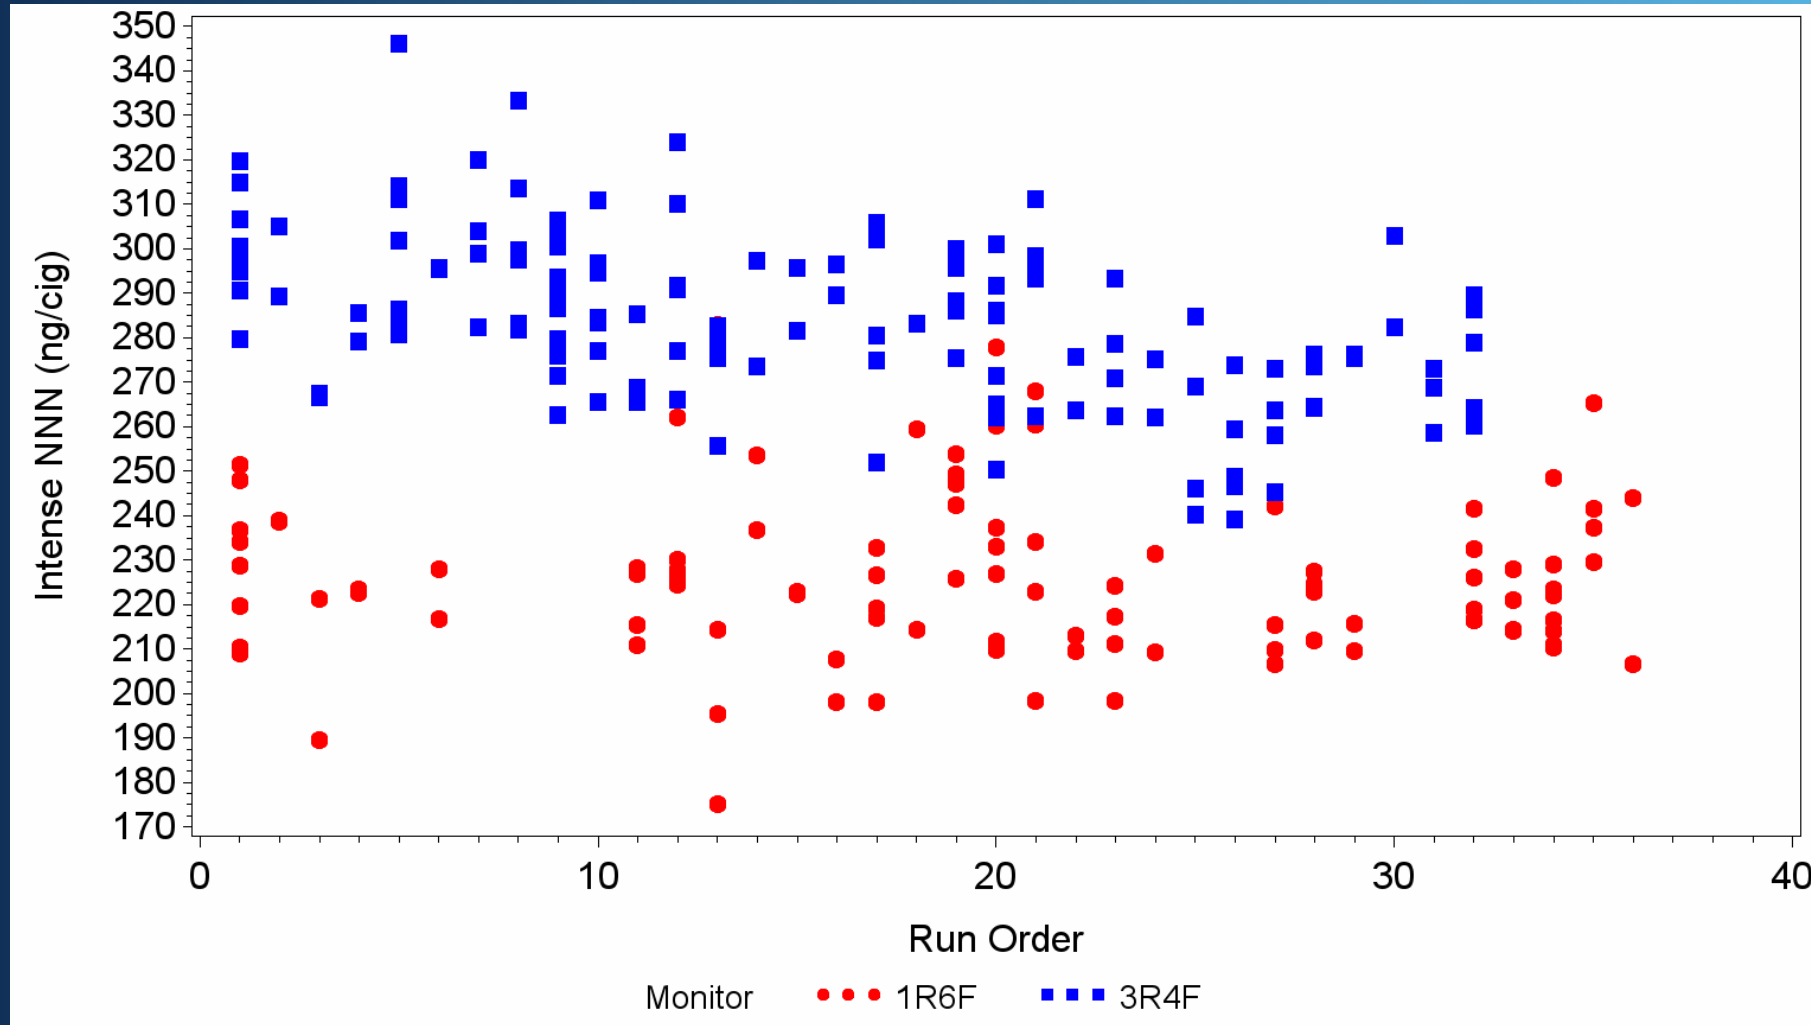


Formaldehyde – Non-Intense

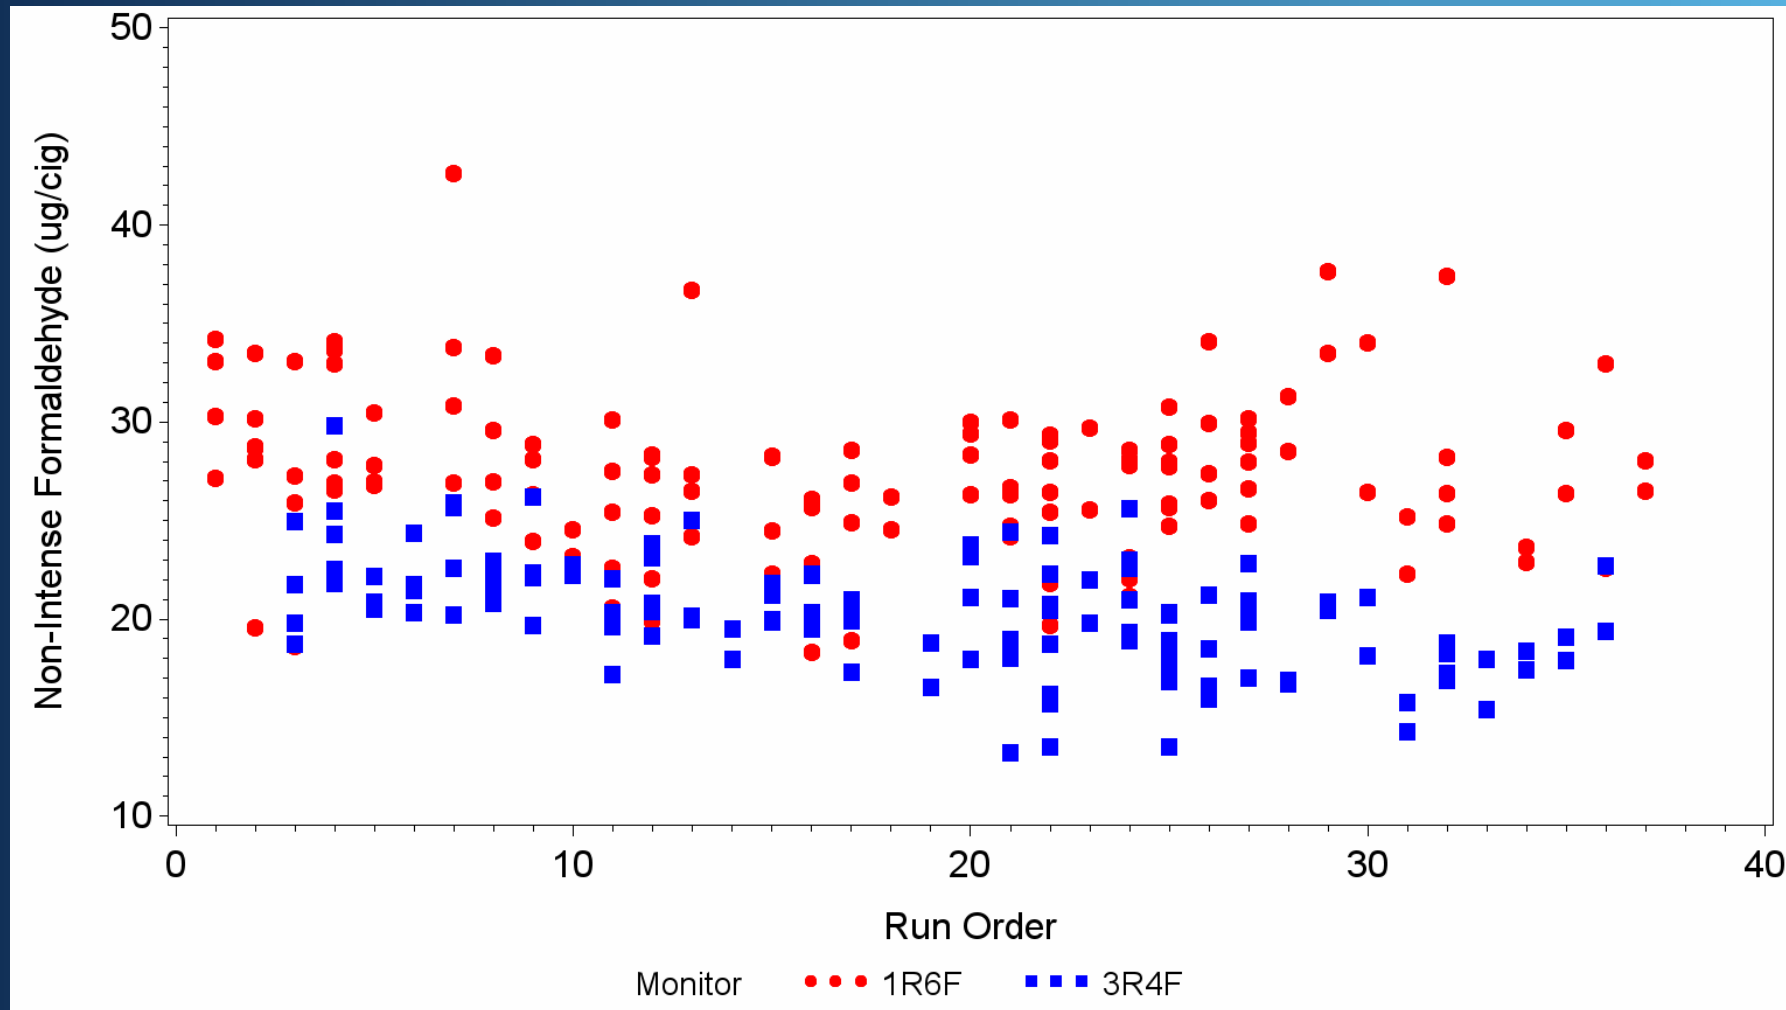

B(a)P – Non-Intense

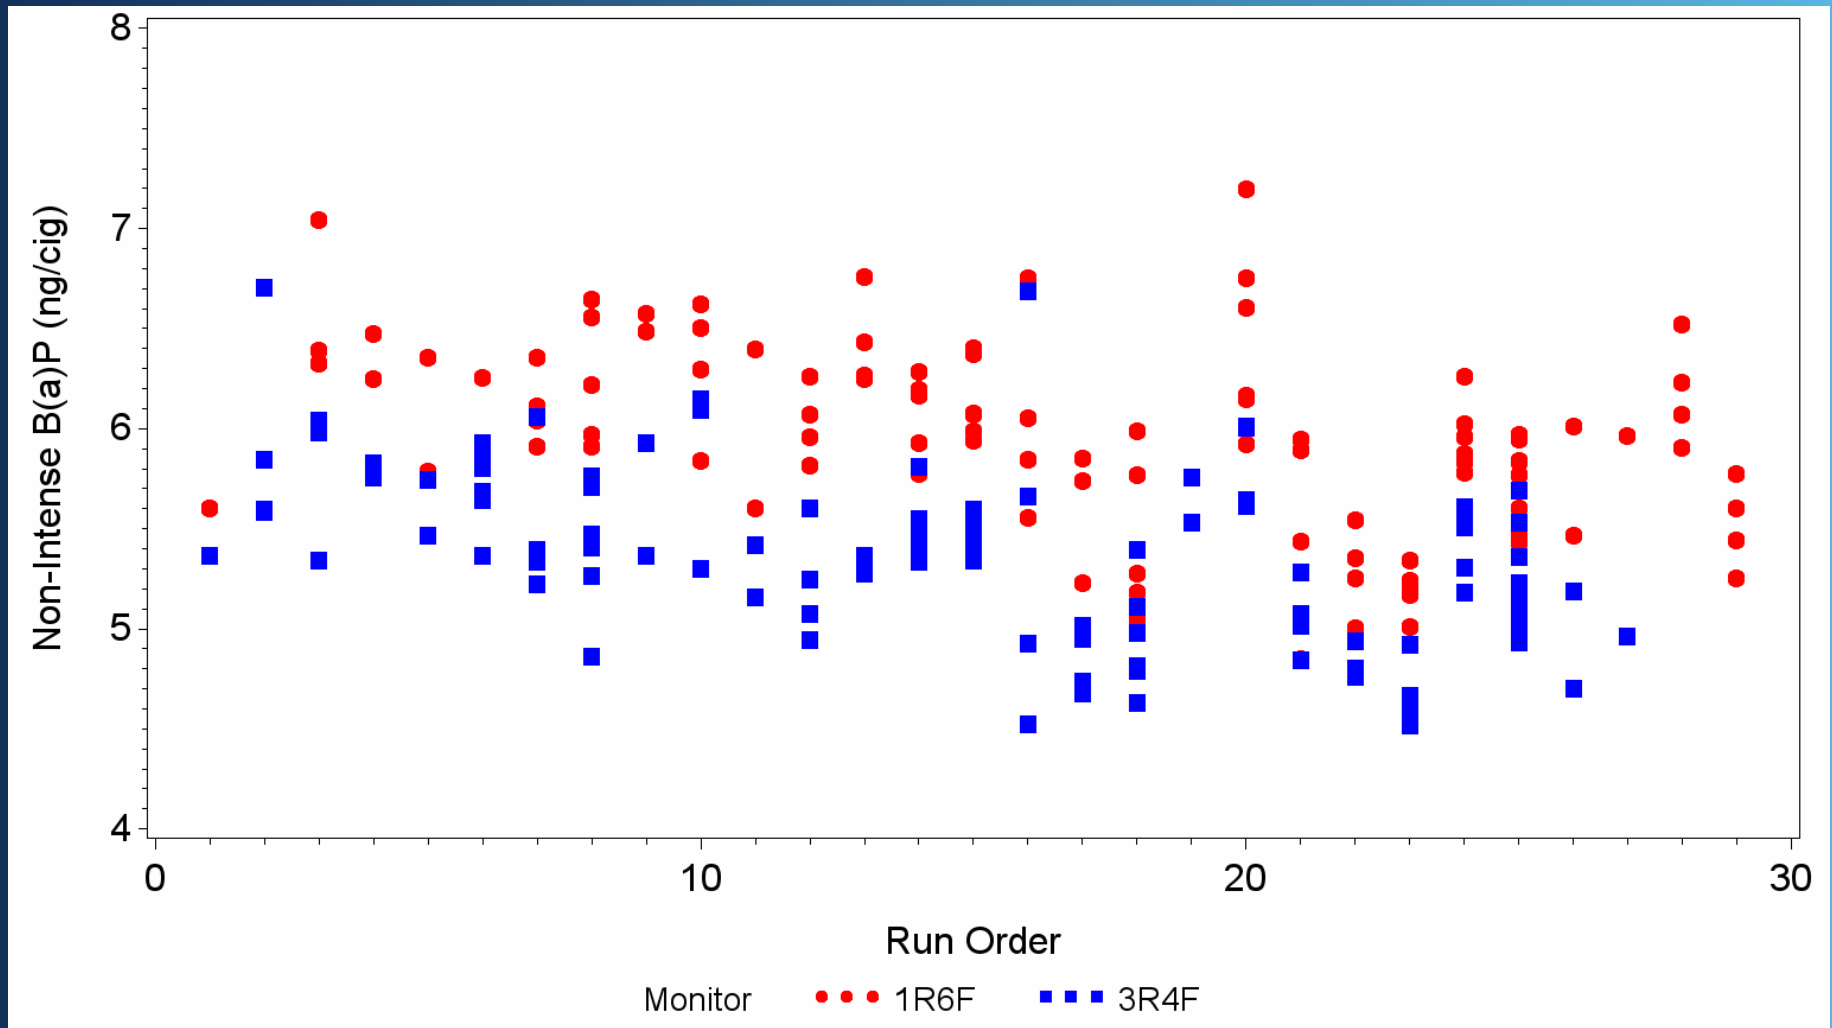

Day-to-day Variance Comparison

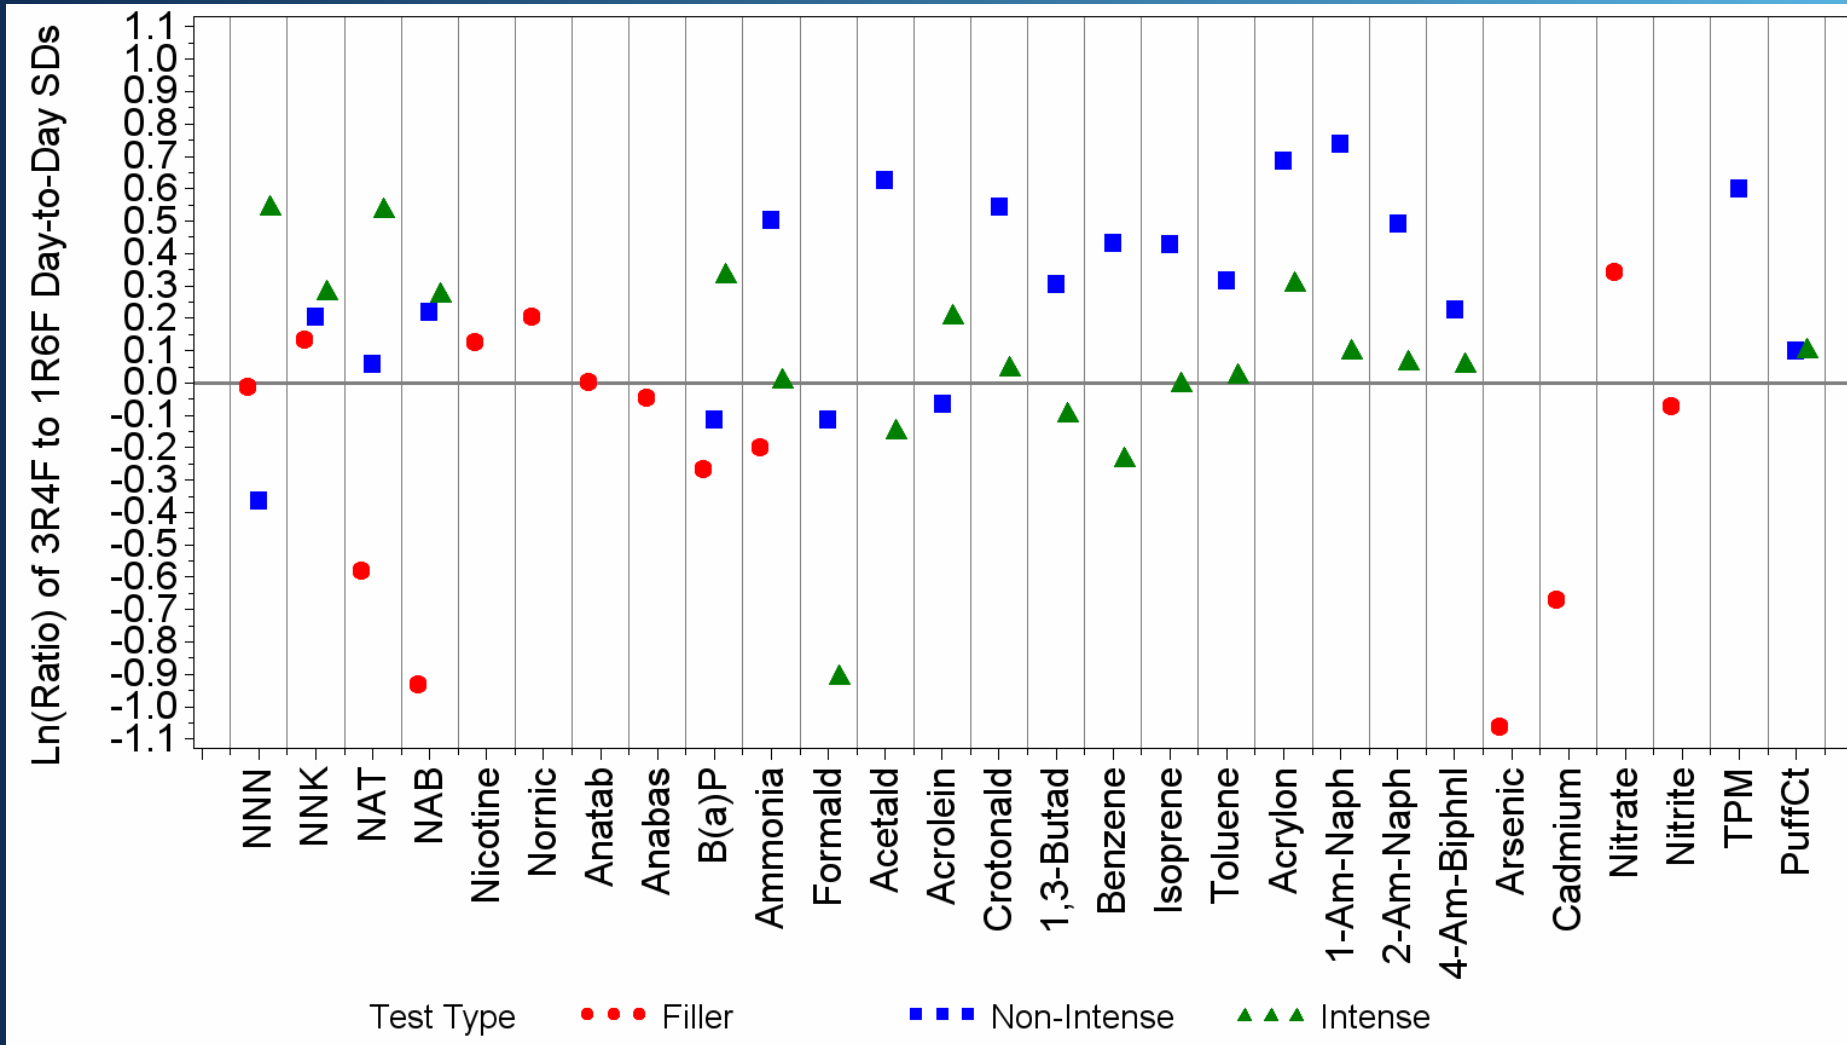


3R4F shows slightly more variability in non-intense smoke results

Overall, there is not a statistically significant difference in variability


1R6F Certified Values

- 1R6F has certified values and certified uncertainty
- The uncertainty around the certified values is intended to represent 95% confidence intervals around the mean value
 - The uncertainty is not intended to represent a 95% prediction interval for individual test results
- The long-term average of results in a lab should normally be within, or very near, the confidence interval, but individual results would be expected to sometimes fall outside the confidence interval

1R6F Averages Compared to Certified Values

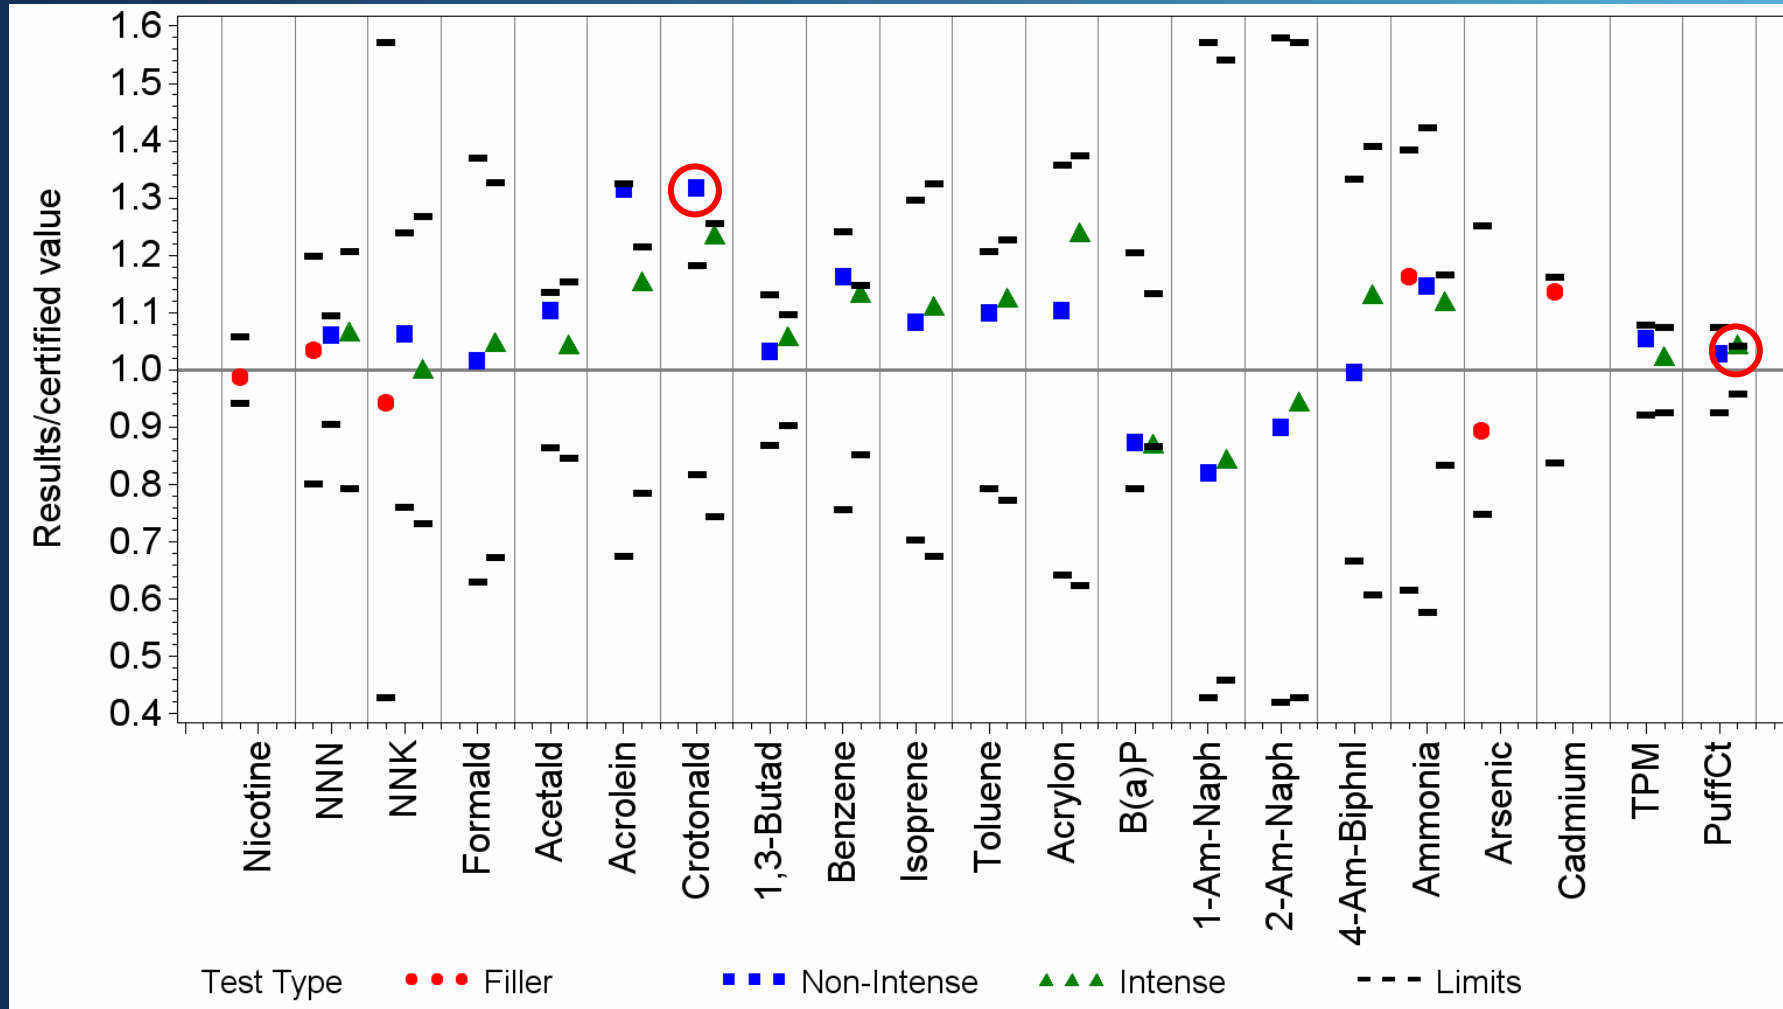

1R6F Individual Results Compared to Certified Values

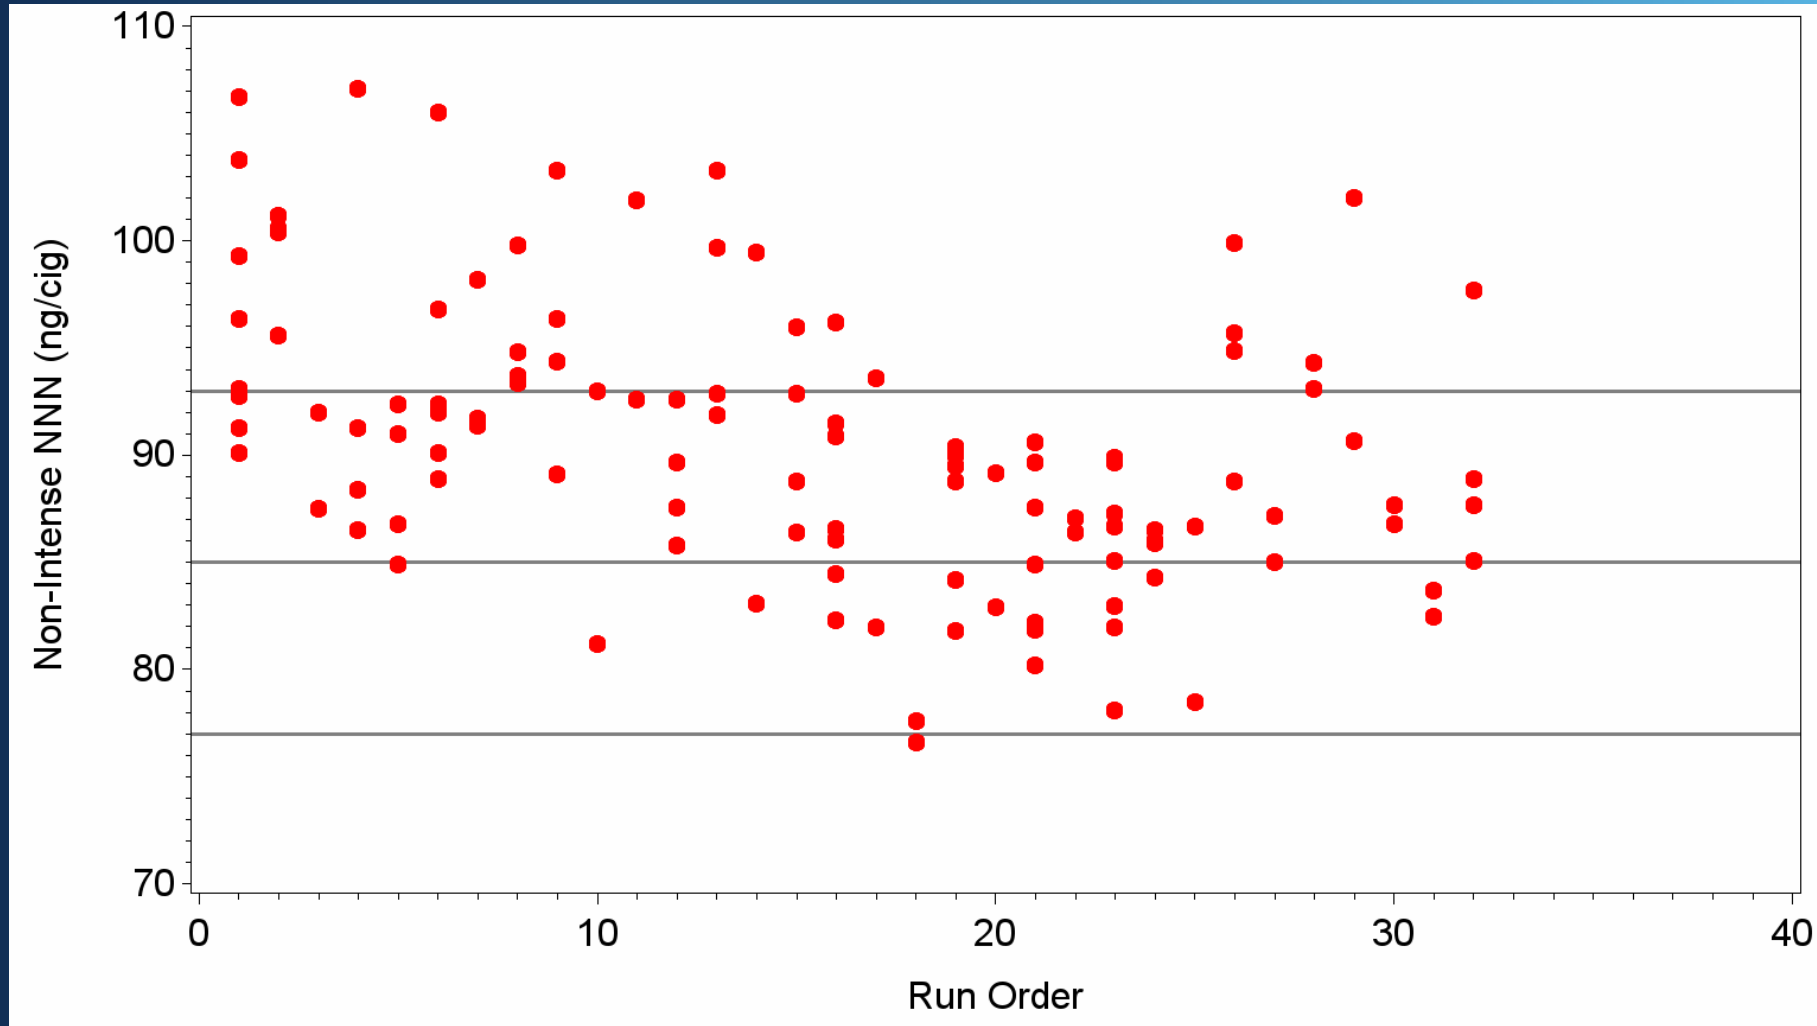

Even if the long-term mean is within the certified uncertainty limits, many individual data points can be outside those limits.

Summary and Conclusions

- A common use of reference cigarettes is as a laboratory QC monitor for method process control
- Our lab carried out this work prior to substituting 1R6F as a lab monitor to replace 3R4F
- There were several analytical differences between the two reference cigarettes, but 1R6F showed similar or reduced variability compared to 3R4F, so is a reasonable replacement.
- The average values of 1R6F in our lab fell within the certified uncertainty (with two exceptions)
- All should understand the certified uncertainty is related to a confidence interval about the mean value, not prediction intervals for individual results



Questions?

THANK YOU



More questions? Email us!
Michael.J.Morton@altria.com
AltriaScience@altria.com

